


REV	ECO	DATE	DESCRIPTION	DB
G	3912	6-Aug-08	ADD BEAM EXIT Ø, CONVERT TO SOLIDWORKS	DMD
H	4107	8-Sep-09	ADD NOTE 5	DMD

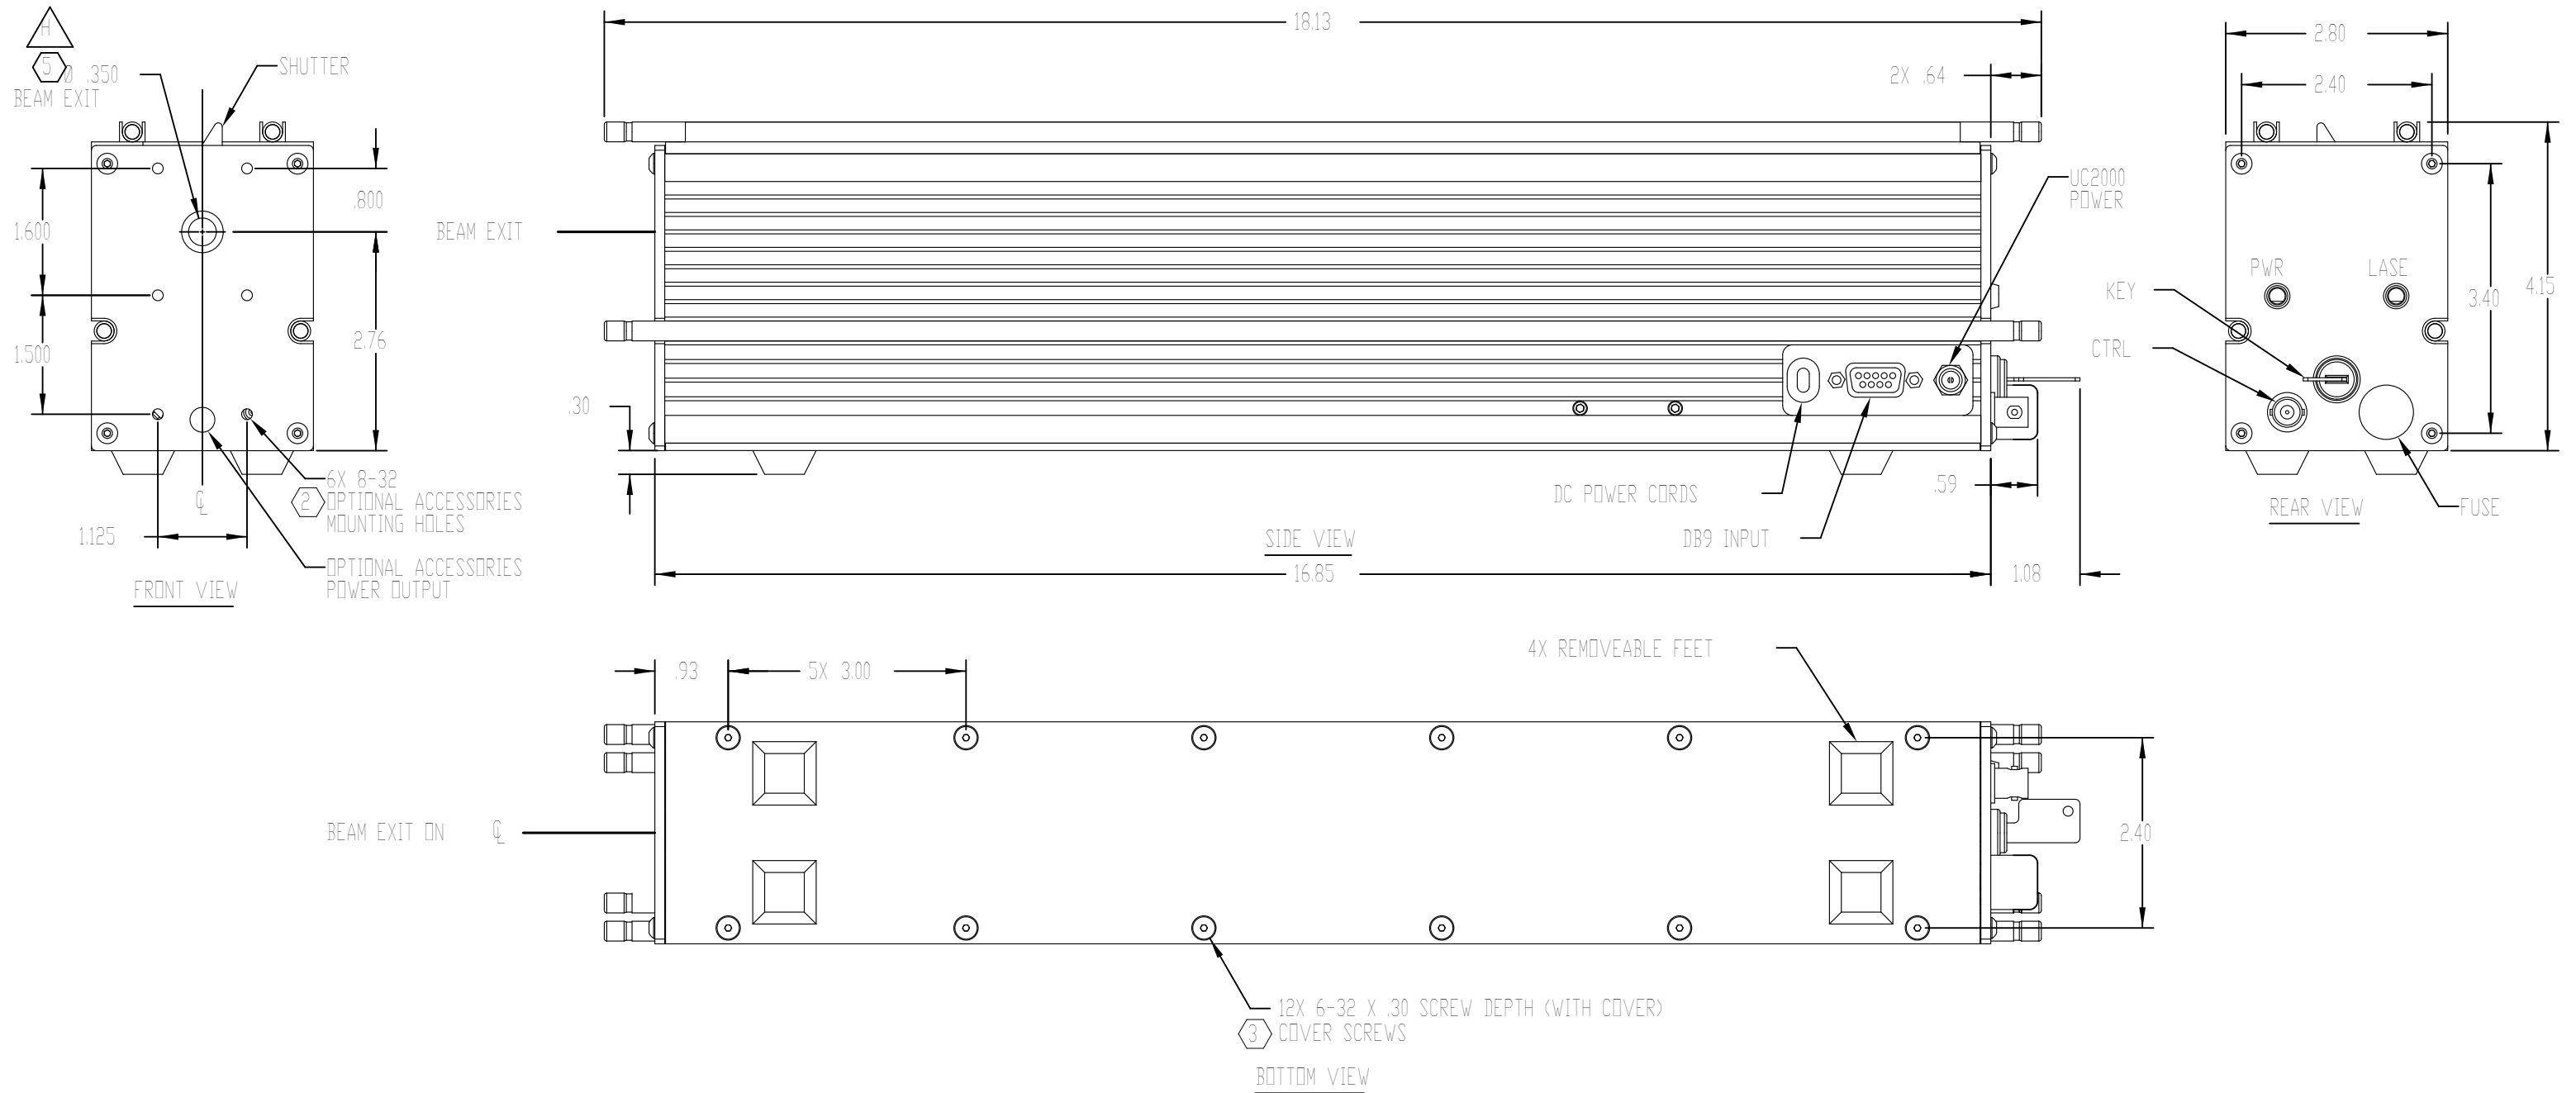

NOTES:

- DO NOT USE COVER SCREW HOLES TO SUPPORT LASER WEIGHT.
- DO NOT USE OPTIONAL ACCESSORIES MOUNTING HOLES TO MOUNT LASER.
- LASER IS MOUNTED BY REMOVING COVER SCREWS AND REPLACING WITH APPROPRIATE LENGTH SCREWS FOR YOUR MOUNTING APPLICATION. USE A MINIMUM OF FOUR SCREWS IN A SYMMETRICAL PATTERN TO PROPERLY DISTRIBUTE MOUNTING FORCES. DO NOT REMOVE COVER.
- WEIGHT: 9 LBS.
- BEAM PATH MAY NOT BE CENTERED OR PERPENDICULAR TO FACEPLATE APERTURE.

TOLERANCES UNLESS NOTED:	
.x = ± 0.1	ANGLE = ± 1°
.xx = ± 0.01	
.xxx = ± 0.005	
MATERIAL:	
FINISH:	

PROPRIETARY THIS DRAWING IS PROPRIETARY TO SYNRAD INC. AND SHALL NOT BE USED OR DISCLOSED IN WHOLE OR IN PART WITHOUT WRITTEN PERMISSION OF SYNRAD INC.	
DESCRIPTION:	
PART NUMBER:	300-16048-01
SHEET	1 of 1
UNITS:	Inches
SIZE:	B

	SYNRAD INC. 4600 Campus Place Mukilteo, WA 98275 Phone: (425)349-3500 Fax: (425)349-3667		
	DESCRIPTION: OUTLINE & MOUNTING, 48-1		
DWG/FILE NUMBER:	300-16048-00	DATE:	19-Feb-96
DRAWN BY:	A. Dexter	CHECKED BY:	
APPROVED BY:		DATE:	